PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION International Bureau



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶:

A61B 17/22

A1

(11) International Publication Number: WO 99/35979

(43) International Publication Date: 22 July 1999 (22.07.99)

(21) International Application Number: PCT/US98/26938

MAN TO A STATE OF THE STATE OF

(22) International Filing Date: 18 December 1998 (18.12.98)

(30) Priority Data:

09/006,563

13 January 1998 (13.01.98)

US

(63) Related by Continuation (CON) or Continuation-in-Part (CIP) to Earlier Application

US Filed on 09/006,563 (CON) 13 January 1998 (13.01.98)

(71) Applicant (for all designated States except US): LUMEND, INC. [US/US]; 400 Chesapeake Drive, Redwood City, CA 94063 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): SELMON, Matthew, R. [US/US]; 675 Mountain House Road, Woodside, CA 94062 (US). HILL, Richard, E. [US/US]; 2430 Oregon Street, Berkeley, CA 94062 (US). CO, Fred, H. [US/US]; 622 Bucher Avenue, Santa Clara, CA 95051 (US). MILO, Charles, F. [US/US]; 32407 Monterey Drive, Union City, CA 94587 (US). FRENCH, Ronald, G. [US/US]; 555 Bryant Street, Palo Alto, CA 94301 (US).


(74) Agent: ENG, U., P., Peter, Wilson Sonsini Goodrich & Rosati, 650 Page Mill Road, Palo Alto, CA 94304-1050 (US).

(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).

Published

With international search report.

(54) Title: METHODS AND APPARATUS FOR CROSSING TOTAL OCCLUSIONS IN BLOOD VESSELS

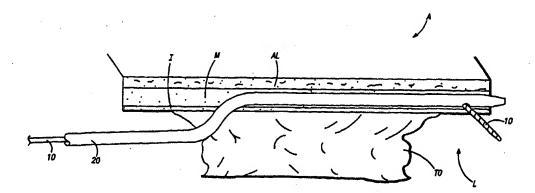

(57) Abstract

Total occlusions are crossed by passing a guidewire or other penetrating wire from a point proximal to the occlusion into a subintimal space between the intimal layer and adventitial layer of the blood vessel wall. The wire is advanced to a point distal the occlusion and thereafter deflected back into the blood vessel lumen, typically using a deflecting catheter which is advanced over the guidewire after it has been positioned within the subintimal space. After the guidewire is returned to the blood vessel lumen, the deflecting catheter may be withdrawn and the guidewire is available for introduction of other interventional and diagnostic catheters.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

ļ.					•		
AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria .	FR.	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina.	GE	Georgia	MD	Republic of Moldova	TG	Togo
· BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN ·	Guinea	MK	The former Yugoslav	TM	Turkmenistan
BF	Burkina Faso	GR	Greece		Republic of Macedonia	TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus .	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's	NZ	New Zealand		
CM	Cameroon		Republic of Korea	PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		•
DE	Germany	LI	Liechtenstein	SD	Sudan		·
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	- LR	Liberia	SG	Singapore		

15

20

25

30

35

METHODS AND APPARATUS FOR CROSSING TOTAL OCCLUSIONS IN BLOOD VESSELS

BACKGROUND OF THE INVENTION

1. Field of the Invention

The present invention relates generally to medical devices, kits, and methods. More particularly, the present invention relates to systems and procedures for crossing chronic total occlusions in blood vessels with guidewires and subsequently performing angioplasty, atherectomy, stenting, or other treatments.

Cardiovascular disease is a leading cause of mortality worldwide. Cardiovascular disease can take many forms, and a variety of specific interventional and pharmaceutical treatments have been devised over the years with varying levels of success.

A particularly troublesome form of cardiovascular disease results when a blood vessel becomes totally occluded with atheroma or plaque, referred to as a chronic total occlusion. Until recently, chronic total occlusions have usually been treated by performing a bypass procedure where an autologous or synthetic blood vessel is anastomotically attached to locations on the blood vessel upstream and downstream of the occlusion. While highly effective, such bypass procedures are quite traumatic to the patient.

Recently, catheter-based intravascular procedures have been utilized to treat chronic total occlusions with increasing success. Catheter-based intravascular procedures include angioplasty, atherectomy, stenting, and the like, and are often preferred because they are much less traumatic to the patient. Before such catheter-based treatments can be performed, however, it is usually necessary to cross the occlusion with a guidewire to provide access for the interventional catheter. In some instances, crossing the occlusion with a guidewire can be accomplished simply by

10

15

20

25

30

35

pushing the guidewire through the occlusion. The guidewire remains in the blood vessel lumen and provides the desired access path. In many cases, however, the guidewire inadvertently penetrates into the subintimal space between the intimal layer and the adventitial layer of the blood vessel as it attempts to cross the occlusion. Once in the subintimal space, it is very difficult and in many cases impossible to direct the guidewire back into the blood vessel lumen. In such cases, it will usually be impossible to perform the catheter-based intervention and other, more traumatic, procedures may have to be employed.

For these reasons, it would be desirable to provide methods, kits, and apparatus which facilitate crossing a chronic total occlusion in a blood vessel with a guidewire. In particular, it would be desirable to provide catheters, guides, or other apparatus which could be used with a conventional or specialized guidewire to direct or redirect the guidewire from the subintimal space back into the blood vessel lumen after the guidewire has entered such space. Such methods and apparatus should be useful in coronary arteries as well as other blood vessels and should be capable of being performed with or without imaging from within or adjacent to the blood vessel. The apparatus for achieving these objective should be of simple construction and be capable of being used in a straight-forward, generally fool-proof manner. At least some of these objectives will be met by the invention described hereinafter.

2. Description of the Background Art

Catheters having side guidewire entry ports spaced proximally from their distal tips are described in U.S. Patent Nos. 5,464,395; 5,413,581; 5,190,528; 5,183,470; 4,947,864; and 4,405,314. Catheters and methods for forming lateral penetrations through tissue to and from blood vessels past total occlusions are described in U.S. Patent Nos. 5,443,497; 5,429,144; 5,409,019; 5,287,861; WO 97/13463; and WO 97/13471.

10

15

20

25

30

35

3

PCT/US98/26938

SUMMARY OF THE INVENTION

According to the present invention, methods are provided for crossing total occlusions in blood vessels. While the methods are particularly beneficial for the treatment of coronary artery disease, they are also useful in the treatment of other arteries and veins, such as the treatment of peripheral vascular diseases.

The total occlusions are crossed by first forming a track from a lumen in the blood vessel into a subintimal space between an intimal layer and an adventitial layer of the blood vessel. The track is formed so that it extends from a location proximal of the total occlusion to a location which is distal to the total occlusion. A passage is then formed from the track back into the blood vessel lumen at the distal location. In the specific embodiments, the track is formed by advancing a wire through the blood vessel lumen into the subintimal space, typically by advancing the wire until it encounters the total occlusion. By continuing to advance the wire, it will usually pass into the subintimal space and can be further advanced to the desired distal location. After the wire is located distally to the total occlusion, it is typically deflected from the track back into the blood vessel lumen.

In the exemplary methods, the wire is deflected using a deflecting catheter. Typically, the deflecting catheter is advanced over a proximal end of the wire and advanced into the track within the subintimal space. and the deflecting catheter are then manipulated so that the wire is deflected laterally through the intimal layer back into the blood vessel lumen. Such deflecting catheters are also useful in supporting the wire as it is advanced into and/or through the track, i.e. the catheter can enhance the "pushability" of the wire when it is advanced forward through any resisting material. Specific designs for such deflecting catheters are described in detail below. Alternatively, the wire which is initially positioned within the track in the subintimal space may be withdrawn through the deflecting catheter and exchanged for a second wire or other device

WO 99/35979 PCT/US98/26938

suitable for penetrating through the intimal layer back into the blood vessel lumen. It will be appreciated that the wires and/or deflecting and other catheters may be freely exchanged over or through one another in a conventional matter without departing from the present invention.

5

10

15

20

25

30

35

It will usually be necessary to determine when the wire and/or deflecting catheter are positioned distal to the total occlusion so that the wire may be returned to the blood vessel lumen beyond said occlusion. Most simply, such position determination can be made by fluoroscopically imaging the blood vessel in a conventional manner. Alternatively or additionally to such fluoroscopic imaging, intravascular imaging, e.g. intravascular ultrasonic imaging (IVUS), and a variety of optical imaging modelities, such as optical coherence tomography (OCT), may be employed. For example, an ultrasonic imaging guidewire may be used to initially access the subintimal space and/or may be exchanged for the wire which is used to access the subintimal space. An imaging guidewire present in the subintimal space may readily detect the presence or absence of occluding material within the blood vessel lumen. When the transition from occluding material to lack of occluding material is detected, it is known that the position of the guidewire has advanced beyond the total occlusion.

After the passage is formed back from the track into the blood vessel lumen and a wire is in place across the total occlusion, the wire is available for use as a guidewire in positioning interventional and diagnostic catheters across the total occlusion. Most commonly, interventional catheters will be positioned across the total occlusion for treating the occlusion. Exemplary interventional catheters include angioplasty balloon catheters, rotational atherectomy catheters, directional atherectomy catheters, stent-placement catheters, and the like.

In a preferred aspect of the methods of the present invention, the wire deflecting step will comprise deflecting a cannula from the subintimal space back into the blood vessel lumen and thereafter passing the wire through a path defined

10

15

20

25

30

35

by the cannula, typically by a lumen within the cannula. Usually, the cannula will be advanced over the wire after the wire is disposed within the subintimal space, and the cannula-deflecting step will comprise advancing a resilient (preformed) curved end of the cannula from a constraining lumen into the blood vessel lumen. Alternatively, the wire-deflecting step may comprise advancing a deflecting catheter over the wire which has been advanced into the subintimal space. A cannula may then be advanced through a lateral opening of the deflecting catheter and penetrated through the intimal layer to define a path for the wire back into the blood vessel lumen. Steerable and other actively deployed cannulas may also be used.

The present invention further provides kits comprising a wire-deflecting catheter having a lumen or mechanism capable of laterally deflecting a wire. will further comprise instructions setting forth any of the methods described above. Optionally, the kit may further comprise the wire which is used for penetrating the subintimal space and/or back into the blood vessel lumen. The kit will usually still further comprise a package for containing both the wire deflecting catheter and the instructions, and optionally the additional wire(s). Suitable packages include pouches, trays, tubes, boxes, and the like. The instructions may be printed on a separate package insert or may be printed in part or in whole on the packaging itself. Usually, the components of the kit within the package will be sterilized by conventional procedures.

Apparatus according to the present invention comprise wire-deflection systems. Exemplary wire-deflection systems usually comprise the wire-deflecting catheter which includes a catheter body and a deflecting cannula. The catheter body will have a proximal end, a distal end, and at least one lumen extending through at least a distal portion thereof. The lumen will have a distal opening and a lateral opening. The cannula also has a proximal end, a distal end, and at least one lumen extending through a distal portion thereof. The distal portion of the cannula will have a pre-

10

15

20

25

30

35

formed, resilient curve. The cannula will be slidably disposed within the lumen of the catheter body to assume (a) a straightened configuration when the cannula is proximally retracted within the catheter body lumen and (b) a curved configuration when the cannula is extended laterally through the lateral opening of the catheter body. In this way, the cannula can be selectively deflected through the intimal layer of the blood vessel according to the preferred methods described above. The system may further comprise a wire configured to pass through the cannula lumen. The wire may be a conventional guidewire, but will more typically be a wire having a sharpened distal tip intended particularly for penetrating the intimal layer of the blood vessel wall. Optionally, the wire may further comprise an imaging means such as an ultrasonic imaging means. The catheter body will. typically have a fluoroscopically visible marker near its distal end. The marker will be configured to permit visual determination of the rotational orientation of the distal end of the catheter body when viewed in a two-dimensional fluoroscopic image. The catheter body will usually be reinforced to enhance torsional rigidity, and may further comprise a distal nose cone wherein the distal and lateral openings are defined within the nose cone. The distal end of the cannula will usually be pre-formed in a smooth curve which may extend over an arc in the range from 15° to 135°, usually from 45° to 90°. The pre-formed curve may have a radius in the range from 0.5 mm to 15 mm, usually from 2 mm to 10 mm.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is a schematic illustration of a coronary artery showing the intimal layer, the medial layer, and the adventitial layer.

Fig. 2 is a schematic illustrations of a total occlusion within the coronary artery of Fig. 1, shown in full section.

Figs. 3A-3D illustrate the method of the present invention for crossing a total occlusion with a wire using a deflecting catheter.

10

20

30

35

PCT/US98/26938

Figs. 3BB illustrates an alternate guidewire advancement step for the method of Figs. 3A-3D.

Fig. 4 illustrates a first embodiment of the distal end of a deflecting catheter suitable for use in the methods of the present invention.

Fig. 5 illustrates a second embodiment of the distal end of a deflecting catheter useful in the methods of the present invention.

Fig. 6 illustrates a third embodiment of the distal end of a deflecting catheter useful in the methods of the present invention.

Fig. 7 illustrates a presently preferred embodiment for the wire-deflecting catheter and system of the present invention.

Figs. 8 and 9 are detailed, cross-sectional views of the distal end of the catheter of Fig. 7, illustrating an internal cannula in a retracted and advanced configuration, respectively.

Fig. 10 is a schematic illustration of a proximal hub of the catheter of Fig. 7.

Figs. 11A and 11B illustrate a configuration for rotationally keying the proximal end of the catheter of Figs. 7-10.

Fig. 12 illustrates a configuration for rotationally keying the distal end of the catheter of Figs. 7-10.

DESCRIPTION OF THE SPECIFIC EMBODIMENTS

Referring to Fig. 1, a normal (non-diseased) artery A comprises an arterial wall having a number of layers. The innermost layer is referred to herein as the intimal layer I which includes the endothelium, the subendothelial layer, and the internal elastic lamina. A medial layer M is concentrically outward from the intimal layer, and an adventitial layer AL is the outermost layer. Beyond the adventitial layer AL lies the extravascular tissue. As used hereinafter, the region between the intimal layer I and the adventitial layer AL, generally including the medial layer M, will be referred to as the subintimal space. It is the

10

15

20

25

30

35

subintimal space through which the wires, deflecting catheters, and other catheter of the present invention will pass when crossing a total occlusion.

Referring now to Fig. 2, a total occlusion TO within the artery A is illustrated. Total occlusion TO may comprise atheroma, plaque, thrombus, and/or other occluding materials normally associated with cardiovascular disease. By "total" occlusion, it is meant that the occluding material occludes substantially the entire lumen L of the artery or other blood vessel so that blood flow through the vessel is substantially The present invention will usually be used with patients where the totally occluded artery is not immediately life threatening since the tissue distal to the occlusion will receive oxygenated blood from collateral arteries. Usually, however, the blood supply will be insufficient and it will be desirable to treat the occlusion by an intravascular intervention, such as angioplasty, atherectomy, stenting, or the like, to restore blood flow through the affected vessel.

The method of the present invention will be described with reference to Figs. 3A-3D. These figures represent an upper portion of the artery of Fig. 2. As seen in Fig. 3A, a wire 10 is advanced through the lumen of the artery until it encounters the total occlusion TO. time, it is possible that the wire 10 will advance through the occlusion without deflecting into the blood vessel wall. Should that occur, subsequent repositioning of the guidewire according to the methods of the present invention may not be necessary. More usually, however, the wire 10 will advance into the subintimal space within the medial layer M, as shown in Fig. 3A. The intimal layer I and adventitial layer AL together define a "tissue plane" through which the wire will naturally pass as the wire is pushed distally from its The wire 10 will continue to advance until its proximal end. tip passes beyond the distal end of the total occlusion TO, as shown in Fig. 3B. The tip could axially advance well beyond the total occlusion until advancement is ceased.

Fig. 3B shows the guidewire 10 advancing without support. In some instances, however, the guidewire 10 may

10

15

20

25

30

35

encounter significant resistance as it enters and/or passes through the space between the intimal layer I and adventitial layer AL. If resistance is encountered, the deflection, catheter 20 may be used to support and enhance the "pushability" of the guidewire 10 by advancing the catheter to a location just proximal of the distal tip of the guidewire, as shown in Fig. 3B. The guidewire 10 and catheter 20 may then be advanced sequentially, e.g. advancing the guidewire a short distance followed by advancing the catheter, and so on.

According to the present invention, however, once the wire 10 has its distal tip positioned beyond the total occlusion TO, deflecting catheter 20 may be advanced over the wire 10, by coaxial introduction over the proximal end of the wire, until it approaches the total occlusion, also as shown in Fig. 3B. The deflecting catheter 20 is then further advanced over the wire 10 until its distal tip also extends beyond the total occlusion TO, as illustrated in Fig. 3C. deflecting catheter 20 will include some mechanism for laterally deflecting the wire 10 so that it may pass back in a radially inward direction through the intimal layer I back into the blood vessel lumen L. The deflection mechanism may take a variety of forms as described below. As shown in Fig. 3C, a lateral port 22 is provided. The wire 10 may be retracted so that its distal tip lies proximally of the port 22 and then advanced distally so that the wire passes laterally outwardly through the port and back into the blood vessel lumen, as shown in Fig. 3D.

In order to optimize performance of this method, it is usually desirable to assure that the distal tip of the wire 10 and the deflecting port 22 (or other deflecting mechanism) of the deflecting catheter 20 are properly positioned beyond the total occlusion TO without being advanced excessively beyond the end of the total occlusion. Typically, it will be desirable to position the deflecting mechanism at from 0 cm to 2 cm beyond the distal end of the total occlusion TO, preferably from 0 cm to 0.5 cm. As discussed above, such positioning can in some instances be performed using conventional fluoroscopic imaging. For example, in some

15

20

25

30

35

instances it may be sufficient to provide suitable radiopaque markers on the wire and on the deflecting mechanism of the deflecting catheter 20 permitting visual positioning of the tip via fluoroscopy. Often, however, it will be desirable to provide ultrasonic or other imaging at or near the total In one approach, wire 10 may be provided with ultrasonic imaging so that the presence and absence of the occluding material may be detected as the wire is advanced passed the total occlusion TO. Alternatively, the deflecting catheter 20 may be provided with such ultrasonic imaging, e.g. in the form of a phased array located near the distal tip (not shown). Ultrasonic imaging guidewires are described in the patent literature. See, e.g. U.S. 5,095,911, the full disclosure of which is incorporated herein by reference. yet another alternative, an imaging guidewire may be advanced to the region of the total occlusion TO in a direction opposite to that of the wire 10 and catheter 20. In this way, the imaging guidewire need not advance through the total occlusion, but could still detect advancement of the catheter and/or guidewire, particularly if ultrasonically opaque components were provided on either or both of the catheter and In yet another alternative, an ultrasonic imaging catheter or guidewire could be positioned in a vein adjacent to the arterial occlusion site, allowing imaging of the entire occluded region while the guidewire is advanced there through. Other imaging modalities, such as optical coherence tomography (OCT) (see U.S. Patent Nos. 5,321,501; 5,459,570; 5,383,467; and 5,439,000) fluorescence imaging (see U.S. Patent Nos. 4,718,417; and 5,106,387) and Raman spectroscopy (WO 92/18008), may also be employed.

A second desirable feature of the method of the present invention will be rotational positioning of the deflecting catheter 20. It will be appreciated that the direction of deflection is usually selective, and therefore it will be desirable to aim the deflecting mechanism from the subintimal space back toward the arterial or other blood vessel lumen L. If the catheter 22 is provided with ultrasonic imaging, such imaging can be used for rotationally

10

15

20

25

30

35

positioning the distal tip of the catheter. The catheter will be rotationally rigid so that rotation of its proximal end may position the distal end. By then detecting the presence of the blood vessel lumen, the deflecting port 22 or other deflecting mechanism can be properly positioned. In an alternative embodiment, as illustrated below in connection with the exemplary catheter, a rotationally specific fluoroscopic marker may be provided on the catheter 20. The marker will be such that by observing the two-dimensional image of the marker by fluoroscopic imaging, the rotational direction of the catheter tip can be determined.

Referring now to Figs. 4-6, exemplary deflecting mechanisms for the deflecting catheters of the present invention will be described. In Fig. 4, the distal end of the catheter 30 has a distal port 32, a lateral port 34, and a passive deflecting mechanism 36. The catheter 30 may be advanced over the proximal end of a wire so that the wire passes over the deflecting mechanism 36 and back into the main lumen of the catheter 30. The catheter 30 may then be advanced over the wire until the distal tip enters the subintimal space and approaches the distal end of the wire. By retracting the distal end of the wire within the lumen of catheter 30 so that its distal tip is proximal to the deflecting mechanism 36, subsequent distal advancement of the wire will engage the proximal surface of the deflecting mechanism and cause the wire to be deflected laterally through lateral port 34.

A first active deflecting mechanism is illustrated in Fig. 5. There, catheter 40 has a distal port 42 and a lateral port 44. Rather than a passive deflecting mechanism, catheter 40 includes an axially translatable cannula 46 having a resilient, pre-formed distal tip which may be advanced through port 44, as shown in broken line. The cannula 46 has a lumen which provides a guide path for the wire.

Catheter 50 illustrated in Fig. 6 is similar to catheter 40 in Fig. 5, except that no lateral port is provided. Instead, a cannula 52 having a pre-formed distal end may be advanced and retracted out of a distal port 54 of

10

15

20

25

30

35

the catheter 50 so that its distal end can assume a laterally deflected shape, as shown in broken line. It will be appreciated that these three embodiments are intended to be exemplary only. A wide variety of other passive and active deflecting mechanisms could be provided on deflecting catheters for use in the methods of the present invention.

Referring now to Figs. 7-10, a presently preferred exemplary deflecting catheter 100 constructed in accordance with the principles of the present invention will be The deflecting catheter 100 comprises a catheter body 102 having a distal end 104 and a proximal end 106. Catheter body 102 includes a single lumen 108 (Figs. 8 and 9), and a deflecting housing 110 secured to the distal end 104 An actuator hub 112 is secured to the proximal end 106 of catheter body 102, and an axially translatable cannula is disposed within lumen 108. The cannula 114 has a sharpened tip 116, typically formed from a metal, hard plastic, composite, or the like, optically being radiopaque. Alternatively or additionally, it may be desirable to provide at least one separate radiopaque marker or the cannula at or near its distal end to facilitate visualization under fluoroscopic imaging. A distal length 118 of the cannula 114 is pre-formed in a curved shaped, as best seen in Figs. 7 and A rotationally specific radiopaque marker 120 is mounted near the distal end of catheter body 102. As illustrated, the marker has a generally U-shaped configuration so that the rotational position of the distal end of the catheter body 102 will be apparent when the marker is observed in a twodimensional fluoroscopic image.

As with catheter 40 in Fig. 5, the purpose of catheter 100 is to laterally deflect the distal tip of the cannula 114 through a lateral opening 122 in the deflector housing 110. The deflector housing 110 also includes a distal port 124 to permit introduction of the catheter 100 over the proximal end of a guidewire GW, as illustrated in Fig. 8 in broken line. The guidewire GW will pass through the distal port 124 and into the distal end of the cannula 114 and travel through a lumen of cannula 114 all the way to the proximal end

10

15

20

25

30

35

of the catheter 100. The distal length 118 of cannula 114 will be straightened and deflected by axially retracting and advancing the cannula between the configuration shown in Fig. 8 and Fig. 9, respectively.

PCT/US98/26938

Referring now to Fig. 10, the actuator hub 112 comprises a pair of coaxial, telescoping tubes 130 and 132. The outer telescoping tube 132 is connected to a proximal end of cannula 114, typically by an adhesive 134. A proximal fitting 136 is further attached to the proximal end of tube 132 so that the assembly of the cannula 114, tube 132, and fitting 136 will move together as a unit through the hemostatic fitting 140 at the proximal end of the hub 112. Hub 112 further includes a rotational fitting 142 which permits the catheter body 102 to be rotated relative to the hub body. The cannula 114 and catheter body 102 will be rotationally coupled or "keyed" together to limit or prevent relative rotation, typically by keying within the hub and/or near the distal end, so that rotation of the catheter body causes a like rotation of the cannula as the catheter is rotationally positioned within a blood vessel. A side branch 148 is provided on hub 112 to permit perfusion and/or infusion through the lumen 108 of catheter 102.

Keying at the proximal end of the catheter 100 can be achieved in a variety of ways. For example, the telescoping tubes 130 and 132 can be provided with asymmetric, mating peripheral geometries, such as oval cross-sections (Fig. 11A) or triangular cross-sections (Fig. 11B). Keying at the distal end can also be achieved in a number of ways, such as providing the catheter body 102 with an asymmetric lumen 108 and the cannula 114 with a mating cross-section, e.g. a D-shaped cross-section as illustrated in Fig. 12. The ability to limit relative rotation of the cannula 114 within the catheter body 102 is advantageous since it assures that curved distal length 118 is properly oriented (usually directed radially outwardly) when the tip 116 emerges through the opening 122.

In use, catheter 100 will be advanced over guidewire GW while the cannula 114 is retracted, as shown in Fig. 8.

WO 99/35979 PCT/US98/26938

5

10

15

20

14

Once the catheter is properly positioned, cannula 114 may be distally advanced, as shown in Fig. 9. Distal advancement is achieved by forwardly advancing the sleeve 132 in hub 136 relative to the remainder of the hub 112 so that the cannulas move forwardly within the lumen 108 of catheter body 102. Prior to advancing the cannula, the port 122 will be properly positioned so that it is directed toward the blood vessel lumen by rotating catheter body 102, typically using the rotational hub 142. Conveniently, the physician will observe the marker 120 so that the lateral port 122 will be directed in the proper radially inward direction. After the cannula has been advanced into the blood vessel, the guidewire GW may then be advanced into the lumen, the cannula 114 withdrawn proximally, and the entire catheter assembly then withdrawn from over the guidewire, leaving the guidewire in place for introduction of other interventional and/or diagnostic catheters.

While the above is a complete description of the preferred embodiments of the invention, various alternatives, modifications, and equivalents may be used. Therefore, the above description should not be taken as limiting the scope of the invention which is defined by the appended claims.

WHAT IS CLAIMED IS:

- 1. A method for crossing a total occlusion in a
 2 blood vessel, said method comprising:
 3 forming a track from a lumen in the blood vessel
 4 into a space between an intimal layer and an adventitial layer
- of the blood vessel, said track extending from proximal of the
- 6 total occlusion to past the total occlusion; and
- selectively forming a passage from the track back into the blood vessel lumen at a location distal to the total occlusion.
- 2. A method for crossing a total occlusion, said method comprising:
- forming a track from a lumen in the blood vessel into a space between an intimal layer and an adventitial layer of the blood vessel, said track extending from proximal of the total occlusion to past the total occlusion, and
- deflecting a wire from the track back into the blood vessel at a location distal to the total occlusion.
- 3. A method for crossing a total occlusion in a
 blood vessel, said method comprising:
- advancing a wire through a lumen of the blood vessel into a space between an intimal layer and an adventitial layer
- of the blood vessel to create a track in said space past the
- 6 total occlusion; and
- 7 selectively forming a passage from the track back
- 8 into the blood vessel lumen at a location distal to the total
- 9 occlusion.
- 4. A method for crossing a total occlusion in a blood vessel, said method comprising:
- advancing a wire through a lumen of the blood vessel
- 4 into a space between an intimal layer and an adventitial layer
- of the blood vessel; and

- 6 deflecting a wire from the subintimal space back
- 7 into the blood vessel lumen a location distal to the total
- 8 occlusion.
- 1 5. A method as in any of claims 1 to 4, wherein
- 2 the blood vessel is an artery.
- 6. A method as in claim 5, wherein the artery is a
- 2 --- coronary artery.
- 1 7. A method as in any of claims 1 to 4, further
- 2 comprising performing an interventional or diagnostic
- 3 procedure over a wire disposed in the subintimal space.
- 8. A method as in either claim 2 or claim 4,
- 2 further comprising advancing an interventional or diagnostic
- 3 catheter over the deflected wire from proximal to the
- 4 occlusion, through the subintimal space, back into the blood
- 5 vessel lumen.
- 9. A method as in any of claims 1 to 4, further
- 2 comprising imaging the occlusion and blood vessel lumen to
- 3 identify the location distal to the total occlusion.
- 1 10. A method as in claim 9, wherein the imaging
- 2 step comprising imaging from within the subintimal space or
- 3 blood vessel.
- 1 11. A method as in claim 9, wherein the imaging
- 2 step comprises imaging from a position external to the
- 3 subintimal space and the blood vessel.
- 1 12. A method as in claim 9, wherein the blood
- vessel is a coronary artery and the imaging step comprises
- 3 imaging from a position in a vein adjacent to the coronary
- 4 artery.

5 13. A method as in claim 4, wherein a single wire

- is both advanced into the subintimal space and deflected back
- 7 into the blood vessel lumen.
- 1 14. A method as in claim 4, further comprising
- 2 exchanging a first wire which is advanced into the subintimal
- 3 space for a second wire which is deflected back into the blood
- 4 vessel lumen.
- 1 15. A method as in claim 4, wherein the wire
- 2 deflecting step comprises:
- deflecting a cannula from the subintimal space into
- 4 the blood vessel lumen; and
- 5 passing the wire through a path defined by the
- 6 cannula.
- 1 16. A method as in claim 15, wherein the wire
- 2 deflecting step further comprises advancing the cannula over
- 3 the wire after said wire is disposed within the subintimal
- 4 space and before the cannula is deflected.
- 1 17. A method as in claim 16, wherein the cannula-
- 2 deflecting step comprises advancing a resilient curved end of
- 3 the cannula from a constraining lumen into the blood vessel
- 4 lumen.
- 1 18. A method as in claim 4, wherein the wire
- 2 deflecting step comprises advancing a deflecting catheter over
- 3 the wire which has been advanced into the subintimal space.
- 1 19. A method as in claim 18, further comprising
- 2 passing a cannula thorough a lateral opening of the deflecting
- 3 catheter and penetrating the cannula through the intimal
- 4 layer, wherein the wire is thereafter advanced through a lumen
- 5 of the cannula.
- 20. A method as in claim 19, wherein the wire
- 2 deflecting step comprises:

WO 99/35979 PCT/US98/26938

18

retracting the wire into the cannula lumen before 3

4 the cannula is passed through the lateral opening of the

catheter; and 5

advancing the wire through the cannula after said 6

cannula has been passed through the lateral opening of the 7

8 catheter.

- A method as in claim 19, wherein the deflecting 1 step comprises: 2
- withdrawing the wire from the cannula; and 3
- 4 introducing a second catheter into the cannula and
- through said cannula after said cannula has been passed 5
- through the lateral opening of the catheter. 6
- A method as in either claim 20 or claim 21, 22. 1
- wherein the catheter and cannula are withdrawn from over the 2
- wire after said wire has deflected into the blood vessel 3
- lumen. 4

1

- 23. An improved method for advancing a guidewire 1
- thorough a subintimal space between an intimal layer and an 2 .
- adventitial layer and past a total occlusion in a blood 3
- vessel, wherein the improvement comprises selectively 4
- deploying the guidewire through a passage from the subintimal 5
- 6 space back into the blood vessel lumen.
 - 24. A kit comprising:
- 2 a wire;
- a wire deflector having a lumen which deflects a 3
- 4 wire laterally; and
- instructions setting forth use of the wire deflector 5
- according to any of claims 1 to 4. 6
- 25. A kit as in claim 24, wherein the wire, the 1
- wire deflector, and the instructions are packaged together in 2
- a single container. 3

26. A kit as in claim 24, further comprising a

2 wire.

1 27. A wire deflection system comprising:

a catheter body having a proximal end, a distal end,

and at least one lumen extending through at least a distal

4 portion thereof, wherein said lumen has a distal opening and a

5 lateral opening; and

- a cannula having a proximal end, a distal end, and at least one lumen extending through a distal portion thereof,
- 8 wherein said distal portion has a pre-formed resilient curve
- 9 and wherein said distal portion of the cannula is slidably
- 10 disposed in the lumen of the catheter body to assume (a) a
- 11 straightened configuration with said cannula lumen axially
- 12 aligned within the distal opening of the catheter body when
- the cannula is proximally retracted within the catheter body
- 14 and (b) a curved configuration with the cannula extending
- 15 laterally through the lateral opening of the catheter body
- when the cannula is distally advanced within the catheter
- body.
- 28. A system as in claim 27, further comprising a wire configured to pass through the cannula lumen.
- 29. A system as in claim 27, wherein the wire has a
- 2 sharpened distal tip.
- 1 30. A system as in claim 27, wherein the wire
- 2 comprises means for imaging tissue surrounding the wire.
- 1 31. A system as in claim 27, wherein the cannula
- 2 comprises a self-penetrating distal end.
- 1 32. A system as in claim 31, wherein the self-
- 2 penetrating distal end comprises a sharpened distal tip.
 - 33. A system as in claim 27, wherein the cannula comprises a radiopaque marker near its distal end.

- 34. A system as in claim 27, wherein the catheter body has a fluoroscopically visible marker near its distal end wherein said marker permits visual determination of the
- 4 rotational orientation of the distal end of the catheter body.
- 1 35. A system as in claim 27, wherein the catheter body is reinforced to enhance its torsional rigidity.
- 1 36. A system as in claim 27, further comprising a 2 distal nose cone attached to the distal end of the catheter 3 body, wherein said nose cone defines the distal and lateral
- 4 openings.
- 37. A system as in claim 27, wherein the pre-formed curve in the distal end of the cannula extends over an arc in the range from 15° to 135°.
- 38. A system as in either claim 27 or 37, wherein the pre-formed curve has a radius in the range from 1 mm to 20 mm.
- 39. A system as in claim 27, further comprising a hub rotationally secured to a proximal end of the catheter body.

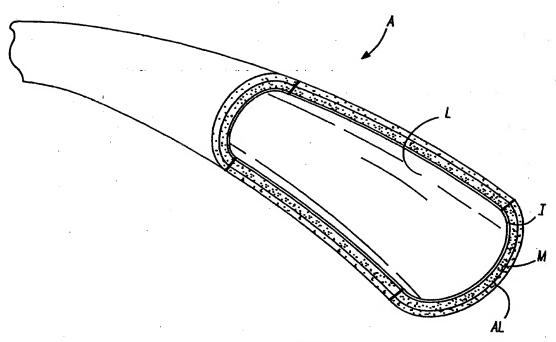


FIG.-1

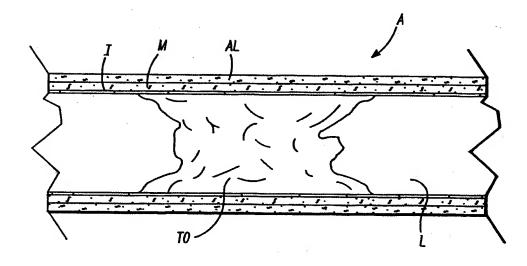


FIG.-2


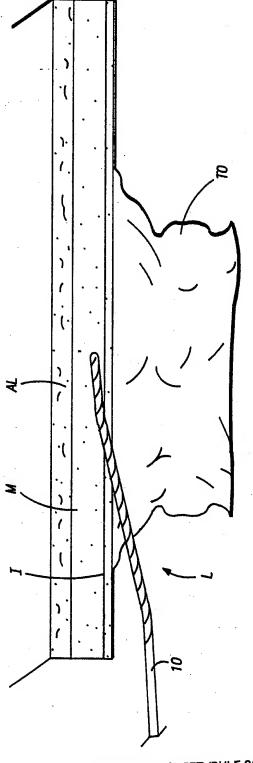



FIG.-3A






SUBSTITUTE SHEET (RULE 26)

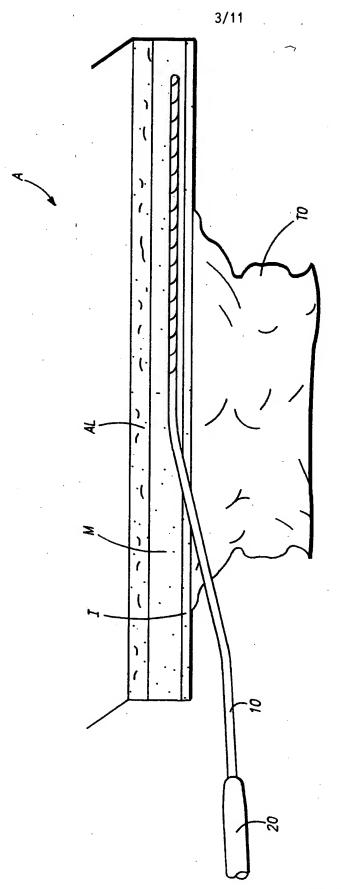

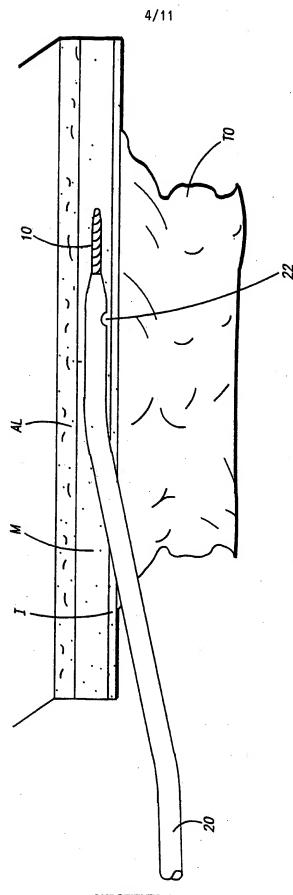

SUBSTITUTE SHEET (RULE 26)



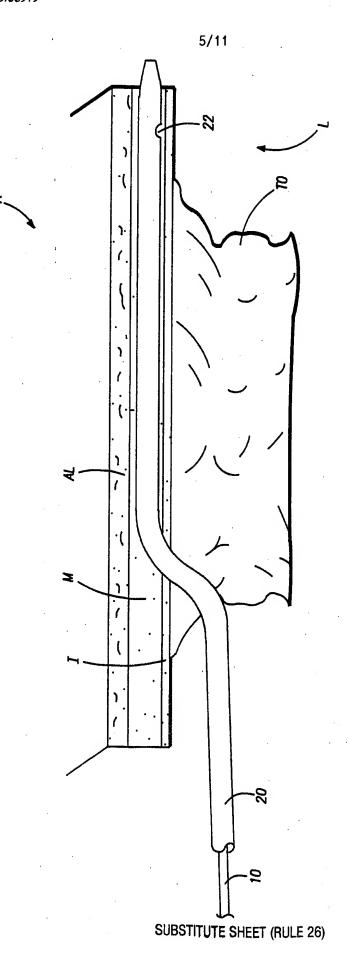

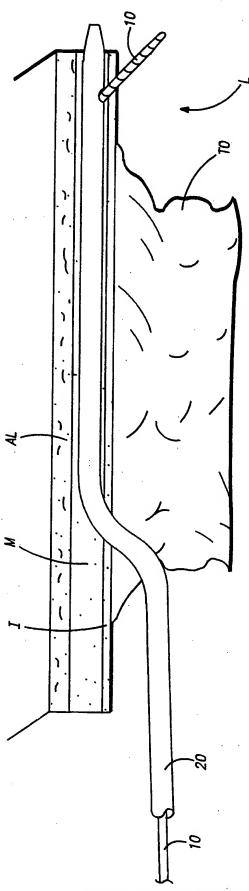


FIG.-3D

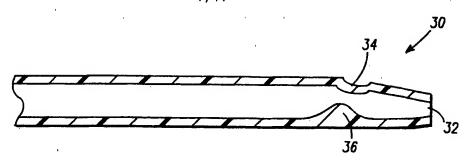


FIG.-4

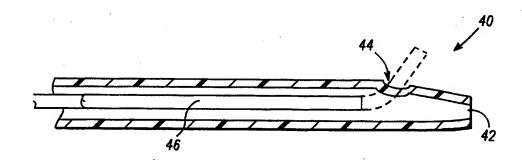


FIG.-5


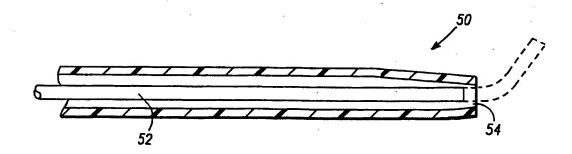


FIG.-6

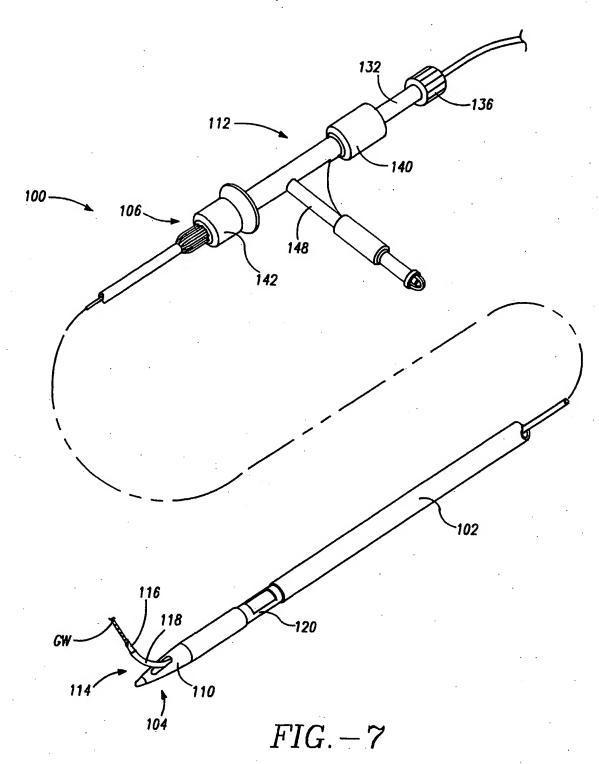

9/11

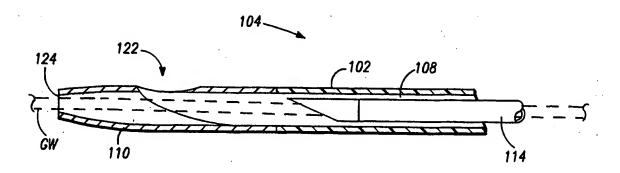


FIG.-8

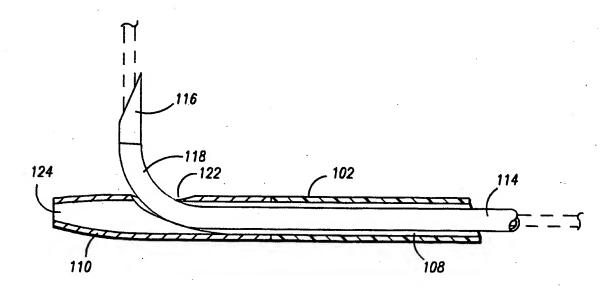


FIG.-9

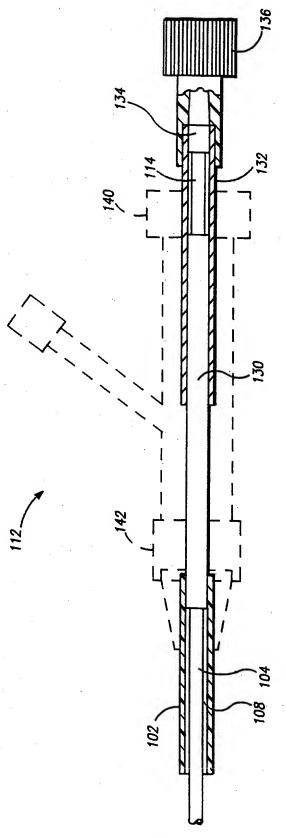


FIG. - 10




FIG.-11A




FIG.-11B




FIG.-12

Intt .onal Application No PCT/US 98/26938

4 40 400			-,
A. CLASS IPC 6	IFICATION OF SUBJECT MATTER A61817/22		
		•	
According to	o International Patent Classification (IPC) or to both national classifi	cation and IPC	
	SEARCHED		
IPC 6	ocumentation searched (classification system followed by classification $A61B$	tion symbols)	*
Documenta	tion searched other than minimum documentation to the extent that	such documents are included in the fields	easmhan
Electronic d	ata base consulted during the international search (name of data b	ase and, where practical search terms us	od)
	*		
C. DOCUM	ENTS CONSIDERED TO BE RELEVANT		
Category °	Citation of document, with Indication, where appropriate, of the re	elevant passages	Relevant to claim No.
X	WO 97 13463 A (TRANSVASCULAR)		24-39
	17 April 1997 cited in the application	•	
	see page 30, line 37 - page 31,	line 35;	
	figure 2A see page 41, line 3 - line 32; f	iauna AA	·
	see page 46, line 3 - line 29	_	4,0
	see page 49, line 3 - page 50, l	ine 21;	
	figures 5A-E see page 57, line 18 - page 59,	line 27:	
٠.	figures 6A,B,I,13A-E	,	
x	US 5 429 144 A (WILK) 4 July 199	5	24-26
	cited in the application		27 20
	see column 6, line 67 - column 7 figures 5A,B	, line 7;	-0.0
	•	-/	•
			, .
Y Furth	er documents are listed in the continuation of box C.	V Retart formits	d In
		X Patent family members are liste	d in annex.
	egories of cited documents : If defining the general state of the art which is not	"T" later document published after the into or priority date and not in conflict with	ternational filing date
conside	nd do he of particular relevance comment but published on or after the international	cited to understand the principle or to invention	heory underlying the
filing da	ate at which may throw doubts on priority claim(s) or	"X" document of particular relevance; the cannot be considered novel or cannot be considered novel or cannot be considered novel.	ot be considered to
, which is	or other special reason (as specified)	Involve an inventive step when the d	claimed invention
	nt referring to an oral disclosure, use, exhibition or	cannot be considered to involve an indocument is combined with one or ments, such combination being obvi	nore other such docu-
"P" documer later the	nt published prior to the international filing date but an the priority date claimed	in the art. "&" document member of the same paten	
Date of the a	ctual completion of the international search	Date of mailing of the international se	
6	April 1999	16/04/1999	
Name and m	alling address of the ISA	Authorized officer	
	European Patent Office, P.B. 5818 Patentiaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,		•
	Fax: (+31-70) 340-2040, 1x. 31 651 apo ni,	Moers, R	•

Inte onal Application No PCT/US 98/26938

C.(Continu	ation) DOCUMENTS CONSIDERED TO BE RELEVANT	00/20930		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.		
A	US 5 628 761 A (RIZIK) 13 May 1997 see abstract; figure 1	29		
A	US 5 695 457 A (ST GOAR FREDERICK G ET AL) 9 December 1997 see column 14, line 27 - line 33	24		
A	WO 97 37581 A (BERTOLERO RAYMOND S; ENDOSCOPIC TECHNOLOGIES INC (US); BERTOLERO A) 16 October 1997 see page 20, line 3 - line 5	24		
4	US 5 095'911 A (POMERANZ MARK L) 17 March 1992 cited in the application see abstract; figure 1	30		
	·			
	•	*		
	* .			
	. 2			
		in the second		
	•			
	·	`		

.. .arnational application No.

PCT/US 98/26938

Box I	Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)
This Inte	ernational Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:
1. X	Claims Nos.: 1-23 because they relate to subject matter not required to be searched by this Authority, namely: Rule 39.1(iv) PCT- Method for treatment of the human or animal body by surgery
2.	Claims Nos.: because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3.	Claims Nos.: because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).
Box II	Observations where unity of invention is lacking (Continuation of item 2 of first sheet)
This Inte	rnational Searching Authority found multiple inventions in this international application, as follows:
1.	As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2.	As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3.	As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4.	No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:
Remark	The additional search fees were accompanied by the applicant's protest. No protest accompanied the payment of additional search fees.

information on patent family members

Inter nal Application No PCT/US 98/26938

Patent document cited in search report		Publication date		Patent family member(s)	Publication date	
WO	9713463	A	17-04-1997	AU	7431696	A 30-04-1997
	-, 10 .00	••	27 0. 2557	AU	7595396	
				CA	2234361	
						- · · · · · ·
				CA		A 17-04-1997
				WO	9713471	
				AU	1847197	A 22-08-1997
				· AU	1847297	A 22-08-1997
		•		AU	1847397	A 22-08-1997
		•		CA	2244066	
	•			CA	2244079	
				CA	2244080	
			•	EP		
					0879068	
		1		WO	9727897	
	•			WO	9727893	
	~=			WO	9727898	A 07-08-1997
US	5429144	Α	04-07-1995	US	5409019	A 25-04-1995
			· .	US	5287861	A 22-02-1995
US	5628761	À	13-05-1997	WO	9601590	A 25-01-1996
US	5695457	Α	09-12-1997	US	5584803	17-12-1996
			•	ΑU	696812 1	
				AU	4284796	
				CA	2206091	
				EP	0841963	
				JP	10510178	
				WO	9617644	
				US	5807318	
			•	US	5558644	
				US	5702368 <i>i</i>	
				US	5766151	16-06-1998
				US	5792094	11-08-1998
				US	5795325	
				ÜS	5769812	
				US	5738652	
				ÜS	5814016	
				US	5868702 /	09-02-1999
WO	9737581	À	16-10-1997	AU	2451197	
				AU	2462597 <i>I</i>	
			·	AU	2665297	29~10~1997
				AU	2666097	
				EP	0892652	
				WO	9737596	
				WO	9737597	
			•	WO	9737597 <i>F</i>	
			17 02 1000			
u2	5095911	Α	17-03-1992	DE	69126890	
				ÐΕ	69126890	
				EP	0591175 /	
				WO	9117710 /	
				ÜS	5558093 /	
				ÜS	5682897 A	
				00	JUGEUSI F	1 UT 11 133/